



Numerical Simulation by Finite Elements for Redistribution of Plantar Pressure in Ergonomic Insoles

Alejandro Rosas Flores and Israel Miguel-Andrés

EasyChair preprints are intended for rapid dissemination of research results and are integrated with the rest of EasyChair.

August 16, 2020

Numerical Simulation by Finite Elements for Redistribution of Plantar Pressure in Ergonomic Insoles

Alejandro Rosas Flores^{1*} and Israel Miguel Andrés^{1†}

¹ Centro de Innovación Aplicada en Tecnologías Competitivas A.C.
arosas.picyt@ciatec.mx, imiguel@ciatec.mx

Abstract

When performing a sport activity there are different factors that influence the practice, including footwear and its components. One of the main components of footwear is the insole, which is responsible for contact with the foot, these can have different purposes, such as: odor control, plantar arch support, reduce pain, humidity control, cushioning, among others. Based on CAE, Finite Element Analysis (FEA) has become a very popular tool thanks to its versatility and accuracy for modeling different footwear components. The aim of this project is to do a numerical simulation by finite element analysis for approve the functionality of ergonomic insoles of different materials that integrate the anthropometric characteristics of the user. The protocols were created to evaluate the baropodometric characteristics with a Baropodometer and a PodoScan2D (Sensor Medica®). The insole was designed using ABAQUS CAE student version and six materials were tested to obtain their mechanical properties using a universal testing machine (Instron), the combination that best redistributes the plantar pressure was found applying this methodology.

1 Introduction

There are different activities that require the use of certain orthotics to reduce or avoid different morphological alterations, the use of ergonomic insoles allows to improve the distribution of plantar pressure and thus avoid deterioration in the structure of the foot and in health in general.

The design and development of ergonomic insoles is a time-consuming process that requires expertise and experience to determine the shape, material, and material thickness, which can lead to trial and error to find a functional product that improves footwear conditions for use. This project aims to carry out a numerical simulation by finite elements that integrates the properties of the material and

* Data analysis and created the first version of this document

† Experimental setup and revision of the document

the anthropometric characteristics of the user for the creation of ergonomic insoles. This document details the theoretical part, experimental part and results.

2 Background

There are different sports in which the athlete puts great efforts on their physical structure, analyzing the foot in sport is essential for the design of orthoses and sport instruments that allow the athlete to improve the practice, the human foot consists of 26 bones and 33 joints; plus muscles and ligaments (Drake, Vogl, Mitchell, & Gray, n.d.). Seven tarsal bones form the ankle as the connection between the leg and the foot, five metatarsals form the medial and lateral areas of the foot, and fourteen phalanges form the toes (Logan et al., 2012). A previous research carried out on Colombian athletes by the biomechanics laboratory of the National Sports School, has determined that there is a tendency to cavus foot in all subjects, regardless of the sport practiced, perhaps caused by the effort required for sports practice (Gómez Salazar et al., 2010). The pes cavus does not absorb as much stress as the flat foot does, but it passes to the tibia and femur. The flat foot absorbs more stress on the musculoskeletal structure of the foot compared to the pes cavus, so the incidence of stress fractures in the foot structure is higher in individuals with flat feet (Frey, 1997). Knowing the anthropometric dimensions allows to create more accurate devices according to the region where they will be used. Reliable anthropometric data and technical ergonomics procedures become powerful tools available today for the optimal dimensional matching of designer products (Ávila Chaurand Rosalío, Prado León Lilia Roselia, & González Muñoz Elvia Luz, 2007). As Smith et al. comment, the use of biomechanics in the design of footwear components provides the resources to know the effects on the lower extremities and find relevant clinical and physical information in order to improve conditions in users (Smith, Wegener, Greene, Chard, & Fong Yan, 2012). In addition to the anthropometric conditions in product engineering, it is necessary to look for materials technology, since they allow obtaining the functional properties that are required for the activity. In an article published by Braithwaite, the importance of materials and their particular use in technical, functional and sensory matters is mentioned, as natural properties of design (Braithwaite, 2017). The choice of the best material for the manufacture of the insole represents what properties the material will provide according to its design, thickness, mechanical properties, etc. So, it is important to define what material will be used. In an article developed by Pratt, Reese and Rodgers analyzed five different materials used for the manufacture of insoles and these were subjected to shock absorption tests, it was found that the viscolas (viscoelastic polymer) is the one that best absorbs impacts (Pratt, Rees, & Rodgers, 1986). One of the problems of the project is to choose the best material for insoles, it seeks to find a material that meets the characteristics to which the product will be exposed during the use, for this the materials engineering allows to identify the mechanical and physical properties of some products through different tests.

The application of the finite element method in the design of the insole will allow to simulate different materials that are subjected to common situations, thanks to this it will be possible to determine if the material and the design of the insole will be able to meet the conditions to which will be exposed.

Assessment different insoles represents a high cost in development, through a finite element analysis it is possible to analyze different designs, materials and situations, different works have been developed that analyzed plantar pressure with insoles developed with polymeric foams (Berroter et al., 2014). The different designs of the insole can affect the way in which the plantar pressure is distributed, depending on the needs of the patient. San Tsung et al., compared the effectiveness of different designs of insole to redistribute the plantar pressure during gait (Tsung, Zhang, Mak, & Wong, 2005). The contact area is important during each of the stages of the gait cycle to determine at which points the plantar pressure is having an effect, in a study developed by Murphy the relationship between the contact area and the plantar pressure was studied (D.F., B.D., J.D., & P.M., 2005).

3 Methodology

To optimize ergonomic design of insoles is necessary to determine the methodology to be followed, with the intention of creating a measurable standardized process to identify key areas of interest to be described and analyzed. The proposed methodology for designing ergonomic insoles, consists in performing the evaluation of the anthropometric characteristics, physical tests, data analysis, development of insoles in CAD, characterization of the material and the numerical simulation by finite elements. Figure 1 shows the methodology for finite element analysis for insoles.

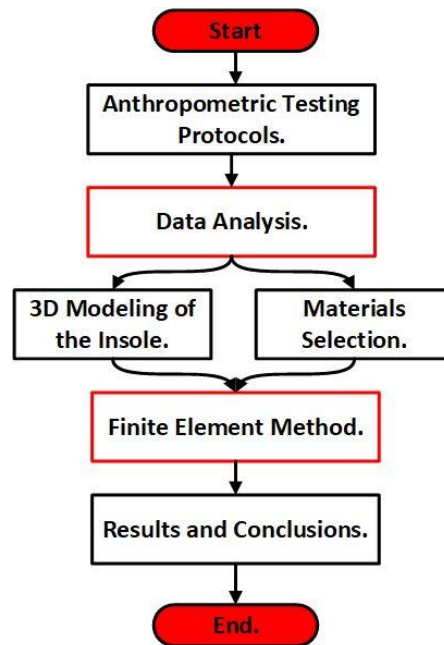


Figure 1: Methodology for finite element analysis for insoles.

3.1 Materials

The procedures, risks and benefits were explained in order to obtain the consent for voluntary participation in writing, in accordance with the General Health Law of Mexico, and considering the principles of the Declaration of Helsinki.

Two equipment were used to take the measurements, a Baropodometer (Sensor Medica®, Guidonia Montecelio, Rome, Italy) that is in charge of taking the plantar pressure tests in its different phases and a 2D PodoScan (Sensor Medica®, Guidonia Montecelio, Rome, Italy) in charge of taking the image of the footprint. Once the operation of the equipment had been explained and the informed consent was signed, the tests were recorded. First, the static test was performed, the user stands at the beginning of the platform barefoot, standing upright with his hands at his sides and the plantar pressure distribution is recorded for 10 seconds. Then the dynamic test took place, the participant was instructed to walk naturally, complete two round-trip cycles and start with the right foot, the execution time of the dynamic test was 30 seconds.

After the tests with the Baropodometer, the patient took a break of 3 minutes to finally perform the scan of the footprint with the PodoScan2D. The participant stood on the PodoScan2D platform with his hands on his sides, the scan was started using the device and the participant was informed when it ended.

3.2 Analysis of biometric test results

Once the anthropometric tests had been done on the equipment, a test report was generated in which important variables were obtained that are used for modeling the insole, this report is automatically generated by the integrated Baropodometer and podoscan2D software. First, a user identification card is generated with general data such as age, weight, height and sex, which were captured by the person in charge at the time of recording the tests. In addition, a detailed summary is generated indicating the main alterations that were detected in the tests. The main values obtained in the study of baropodometry consist of: Contact surface, percentage of the applied load and geometric values. To determine the applied loads that will be applied in the simulation, the foot was divided into six sections where the contact surface in that area is known, as well as the percentage of the load in that area, an example is shown in Figure 2 of the division of the foot.

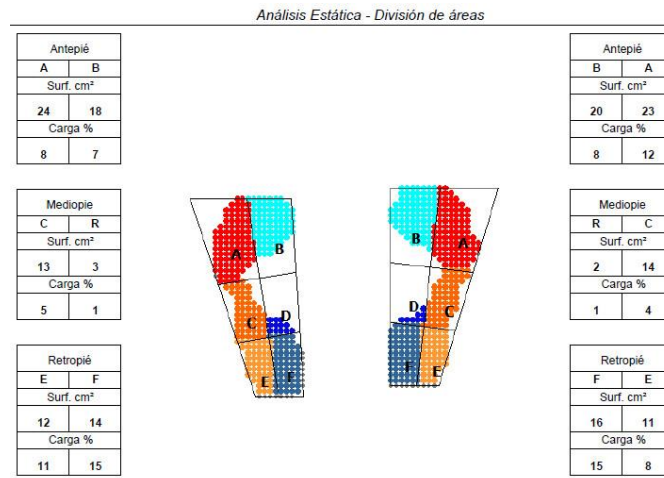


Figure 2: Division of areas of the foot surface.

To determine the load that will be applied in the simulation, the load (mass in kilograms) is multiplied by the distribution of the load in that area and divided by the contact surface, multiplied by the gravity on Earth to obtain the result in Pascals, shows in Equation 1 the procedure to obtain the plantar pressure per section in the foot.

$$Plantar\ Pressure = \left(\frac{m * l}{s} \right) * g$$

Equation 1. Determination of plantar pressure by section.

Where:

m=mass in kilograms

l=percentage of load

s=surface in square meters

g=gravity in meters / square seconds

For the acquisition of the plantar footprint, the PodoScan2D is used, where by scanning the plantar footprint, the digitization of it is obtained, as well as other anthropometric measurements, the Figure 3 shows the acquisition of the plantar footprint as well as its measurements.

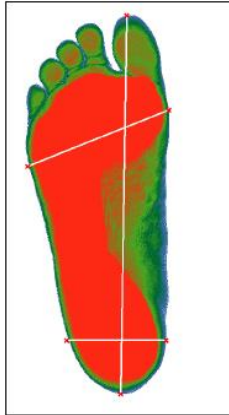


Figure 3: Plantar footprint acquisition using PodoScan2D

3.3 Choice of materials for manufacture

The literature shows that the selection of the material with which the insole is made is based on the orthopedist's preference or their experience, the cost and the availability of resources; for the choice of material, a literature search was done and in the current market analyzing the materials used for redistribution of plantar pressure in different contexts. For the location of the suppliers of these materials, ANPIC (Asociación Nacional de Proveedores de la Industria de Calzado) was visited, the most important supplier fair in the country for the leather-footwear sector organized by CICEG (Cámara de la Industria del Calzado del Estado de Guanajuato) attended by 350 exhibiting companies and more than 11000 buyers and visitors. Table 1 shows the suppliers and the materials that most commercialize for the manufacture of insoles.

Table 1: Suppliers and materials for insole manufacturing

Supplier	Material	Volume(cm ³)	Mass (g)	Density (g/cm ³)
S1	EVA 2.5mm	6.25	0.518	0.083
	EVA 3.0mm	7.5	0.680	0.091
S2	Latex generic	11.25	2.131	0.189
	Latex antibacterial	8	3.411	0.426
	Latex activate carbon	8	2.629	0.329
S3	EVA 3.2mm	8	0.838	0.105

The tensile test was done on the Instron universal testing machine which measures the load supported by the material before breaking. The tests were done under ASTM 638 (Standard Test Method for Tensile Properties of Plastics) and to determine the Poisson's ratio, it was performed under ASTM E132-17 (Standard Test Method for Poisson's Ratio at Room Temperature). Table 2 shows the main results of the tensile test.

Table 2: Results of material tests

Supplier	Material	Young's Modulus (MPa)	Tension Max (MPa)	Deformation Break (%)	Tenacity (MPa)	Tension at break (MPa)	Poisson ν
S1	EVA 2.5mm	1.995	0.833	139.25	0.750	0.833	0.31
	EVA 3.0mm	1.650	0.916	231.55	1.383	0.916	0.29

S2	Latex generic	0.540	0.247	227.88	0.399	0.224	0.11
	Latex antibacterial	0.580	0.312	266.73	0.574	0.310	0.14
	Latex activate carbon	0.561	0.239	218.90	0.366	0.233	0.19
S3	EVA 3.2mm	2.458	1.060	138.45	0.932	1.060	0.36

3.4 Modeling & Simulation

For the modeling of the insole, ABAQUS CAE was used based on the measurements found in the PodoScan2D created from the plantar footprint, in the same way the insole was divided into six sections where the pressures found in the baropodometer will be applied, in the Figure 4 the insole model with its divisions is shown.

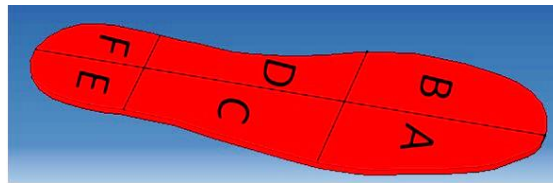


Figure 4: Insole model with its divisions.

Once the insole had been modeled and the mechanical properties of the materials determined, the insole model was meshed, using the type of element "C3D8R: An 8-node linear brick"

To make the comparisons of the deformations of each material, a reference node was created for each foot zone that served as an initial observation point and to determine the deformation in that node. Boundary conditions were applied to limit the displacements and rotations of the insole placed on the ground, and the loads were applied in each of the regions according to the pressures found in the Baropodometer. It is shown in Figure 5 the application of the boundary conditions and applied pressures. Six simulations were done on the left foot and six simulations on the right foot, adapting the characteristics of each material to the model and applying the loads in each region of the foot.

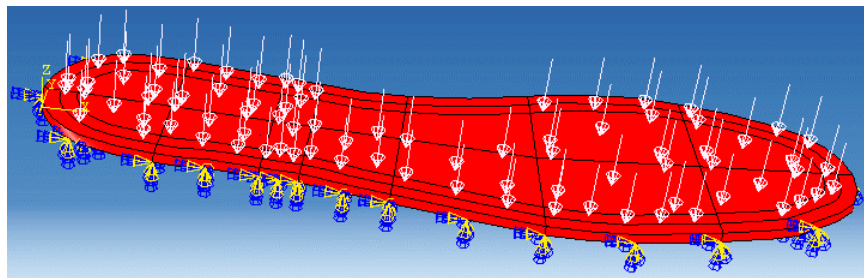


Figure 5: Application of the boundary conditions and applied pressures.

4 Results

Among the main results to be analyzed is the Von Mises stress, it was found that the material that best distributes the plantar pressures is the 3.2 mm thick EVA. Overall, the EVA is superior to latex, in

Figure 6 it can be seen the comparisons of each of the materials analyzed in each foot. Figure 7 shows the right foot insole simulation made from 3.2 mm EVA, during the stresses to which it is exposed during the static phase under normal conditions. The material with the least displacement is the EVA of 3.2 mm thick for the two feet and in each zone. The material with the greatest deformation is the generic 5.5 mm thick latex for both feet and in each area. It is observed that there is a distribution of plantar pressure on the surface of the insole, placing greater effort on the heel.

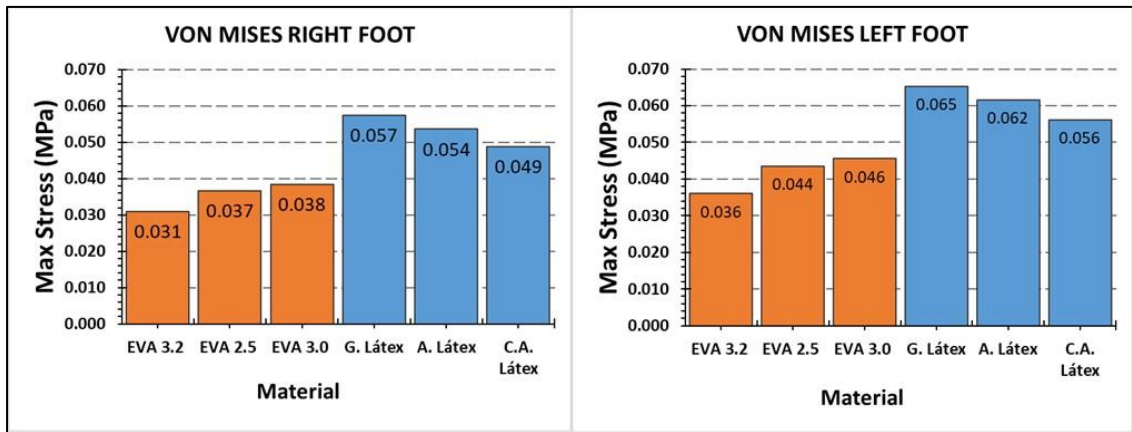


Figure 6: Comparisons of each material

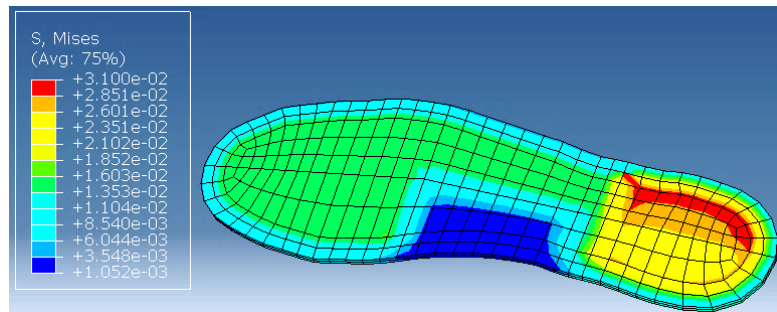


Figure 7: Right foot insole simulation made from 3.2 mm EVA.

5 Conclusions

In relation to the finite element analysis and the mechanical test of the materials, the best material to use is the EVA. It can be observed that EVA has better mechanical properties compared to latex in its different formulations. It is recommended to use EVA from Supplier 3 for the manufacture of ergonomic insoles. The design phase involved the evaluation and analysis of the anthropometric characteristics of the participant to later make the modeling of the insole and perform simulations with different materials, therefore, the objective of performing a numerical simulation by finite element analysis for probing functionality of ergonomic insoles that integrates the materials and the anthropometric characteristics of the user was done and the trial-error time in the elaboration of insoles was minimized.

6 Acknowledgments

Thanks to the Centro de Innovación Aplicada en Tecnologías Competitivas A.C. for the use of spaces and equipment for the development of the project.

References

- Ávila Chaurand Rosalío, Prado León Lilia Roselia, & González Muñoz Elvia Luz. (2007). *Dimensiones antropométricas de la población latinoamericana*. Retrieved from <https://image.slidesharecdn.com/dimantropolatinoam-140922133921-phpapp02/95/dimensiones-antropometricas-latinoamericanas-92-1024.jpg?cb=1411393484>
- Berroter, M., Bol, S., Jose, O., Monrroy, P., Bol, S., Virginia, M., & Simon, C. (2014). *Evaluación numérica por elementos finitos de la redistribución de presiones plantares en plantillas para calzado de personas con pie diabético*. (May 2016).
- Braithwaite, N. (2017). Sensing creativity: The role of materials in shoe design. *Senses and Society*, 12(1), 90–94. <https://doi.org/10.1080/17458927.2016.1223786>
- D.F., M., B.D., B., J.D., M., & P.M., V. (2005). Efficacy of plantar loading parameters during gait in terms of reliability, variability, effect of gender and relationship between contact area and plantar pressure. *Foot and Ankle International*, 26(2), 171–179. Retrieved from http://www.embase.com/search/results?subaction=viewrecord&from=export&id=L40353994;%5Chttp://sfx.ub.rug.nl:9003/sfx_local?sid=EMBASE&issn=10711007&id=doi:&atitle=Efficacy+of+plantar+loading+parameters+during+gait+in+terms+of+reliability,+variability,+eff
- Drake, R. L. (Richard L., Vogl, W., Mitchell, A. W. M., & Gray, H. (n.d.). *Gray's anatomy for students*.
- Frey, C. (1997). *Footwear and stress fractures*. 16(2), 249–257.
- Gómez Salazar, L., Franco Alvarez, J. M., Nathy Portilla, J. J., Valencia Esguerra, E. A., Vargas Bonilla, D. V., & Jiménez Hernández, L. (2010). Características de la huella plantar en deportistas colombianos. *Entramado*, 6(2), 158–167. Retrieved from http://www.unilibrecali.edu.co/images2/revista-entramado/pdf/pdf_articulos/volumen6/volumen6_2/caracteristicas_huella_plantar_deportistas_colombianos.pdf
- Logan, B. M., Sardesai, A. M., Daivajna, S., Robinson, A. H. N., Hutchings, R. T., & McMinn, R. M. H. (Robert M. H. (2012). *McMinn's color atlas of foot and ankle anatomy*. Elsevier/Saunders.
- Pratt, D., Rees, P., & Rodgers, C. (1986). Assessment of some shock absorbing insoles. *Prosthetics and Orthotics International*, 10, 43–45. Retrieved from <http://informahealthcare.com/doi/abs/10.3109/03093648609103079>
- Smith, R., Wegener, C., Greene, A., Chard, A., & Fong Yan, A. (2012). Biomechanics of footwear design. *Journal of Foot and Ankle Research*, 5(S1), 1–2. <https://doi.org/10.1186/1757-1146-5-s1-il>
- Tsung, B. Y. S., Zhang, M., Mak, A. F. T., & Wong, M. W. N. (2005). Effectiveness of insoles on plantar pressure redistribution. *The Journal of Rehabilitation Research and Development*, 41(6), 767. <https://doi.org/10.1682/jrdr.2003.09.0139>